
510(K) SUMMARY OF SAFETY AND EFFECTIVENESS								
1. Applicant/Laboratory Information								
A	A Name Bayer Business Group Diagnostics							
В	B Mailing address 511 Benedict Avenue, Tarrytown, NY 10591							
C	C Phone number 914-631-8000							
D	D Fax number 914-524-2132							
E	E-mail/internet	http://www.bayerdiag.com						
	address							
F	F Contact Kenneth T. Edds, Ph.D., Regulatory Affairs Manager							
2. Regulatory Information								
A	A Class II (assay), I (calibrator)							
В	B Product code 82 LTK (assay), 75 JIT (calibrator)							
C	Classification	Tumor-associated Antigen Immunological test system §866.6010						
	Names Calibrator §862.1150							
D	Common name	Tumor-associated antigen immunological test system						
E	Proprietary name	CA 125 II Assay for the Bayer ADVIA Integrated Module System						
	3. Intended Use(s)/Indication Statement							

The BAYER ADVIA IMS CA 125 II Assay is an in vitro diagnostic device intended to quantitavely measure OC 125 reactive determinants associated with a high molecular weight) glycoprotein in serum of women with primary epithelial invasive ovarian cancer. The CA 125 II Assay is indicated as an aid in the management (monitoring) of ovarian cancer patients when used in conjunction with other diagnostic procedures. The CA 125 II Assay is also indicated as a onetime test for use as an aid in the detection of residual ovarian carcinoma in patients who have undergone first-line therapy and would be considered diagnostic second-look procedures. An assay value of greater than 35 U mL is predictive of residual disease, provided that alternate causes of elevated CA 125 II Assay values can be excluded. It is recommended that the assessment and treatment of patients with ovarian cancer and the use of this CA 125 II Assay be under the order of a physician trained and experienced in the management of gynecologic cancers. This assay is not intended for screening or diagnosis of ovarian cancer or for use on any other system.

4. Substantial Equivalence Information							
A	Predicate device	Bayer Immuno 1 CA 125 II Test					
В	K number	K983715					
C	Comparison with	n with Correlation (Y = ADVIA IMS, X = Immuno 1) [N=45]					
	predicate	• Regression equation = $1.074 (X) - 3.94 = y$					
		• Syx (U/mL) = 13.74					
		• R = 0.994					
		• Sample Range $(U/mL) = 5.1 - 509.2$					
	5. Procedure						

The ADVIA® IMS CA125 II Assay is an *in vitro* heterogeneous sandwich immunoassay using magnetic separation. Reagent 1 (R1) contains a monoclonal antibody to OC 125 labeled with FITC and Reagent 2 (R2) contains a monoclonal antibody to OC 125 conjugated to the enzyme alkaline phosphatase (ALP). The sandwich complex formed by the analyte and the antibody conjugates is captured by the magnetic particles so that the CA 125 11 concentration in the sample can be measured in terms of enzyme activity. The substrate used for this assay is a dioxetane phosphate derivative, which is dephosphorylated by ALP resulting in photon emission. A photomultiplier tube measures luminescence. The dose response curve is proportional to the analyte concentration in sample.

	6. Reagents								
A	Material	 M11 Antibody Conjugate (R1) (Source: Mouse) Alkaline Phosphate-labeled antibody (R2) Monoclonal ImmunoMagnetic Particle (mIMP™) Serum OC 125 determinants [Calibrators] (Source: Mouse) 							
В	Amount	As shipped Concentrations: R1 = 1.5 mg/L; monoclonal OC 125 ALP conjugate = 25.0 mg/L; Sodium Azide = 0.095 % (in each reagent prep), Other (Buffer, surfactant, preservative) Post Assay Concentrations: R1 = 0.08 mg/L; monoclonal OC 125 ALP conjugate = 1.28 mg/L; Sodium Azide = 0.01 %, Other (Buffer, surfactant, preservative)							

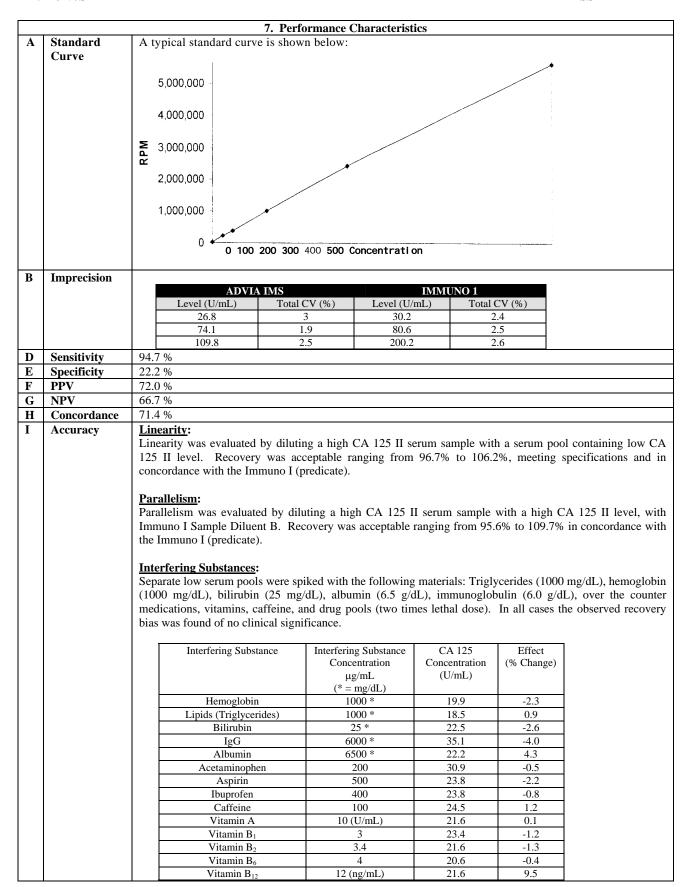

			1				
		Vitamin C	30	24.5	1.4		
		Vitamin D ₂	0.8 (U/mL)	20.6	3.7		
		Vitamin E	0.06 (U/mL)	20.6	2.5		
		Folic Acid	0.8	21.6	7.0		
		Niacin	40	21.6	4.4		
		Vincristine Sulfate	13.5 *	20.6	4.1		
		Vinblastine	5.11 *	20.6	4.1		
		Mitomycin C	73 *	21.6	0.9		
		Tamoxifen – Free	60 *	20.6	4.1		
		Tamoxifen – Citrate	60 *	20.6	4.1		
		Etoposide	415 *	22.5	4.1		
		5-Fluorouracil	1600 *	21.6	3.5		
		Cyclophoshamide Monohydrate	800*	21.6	0.9		
		Doxorubicin HCl	51.8 *	21.6	0.9		
		Diethylstiberol	23 *	20.6	4.1		
		Methotrexate	450 *	22.5	5.6		
		Cis-Platinum	173 *	20.6	4.1		
		Lupron	15 *	25.9	-5.8		
		Megesterol Acetate	243 *	21.6	0.9		
		Hook Effect: On the ADVIA IMS the concentra	ation of up to 80 000 I	I/mL did not prod	luce a signal low	er than the highest	
		calibrator rate (level 6).	ition of up to 60,000 C	mil did not proc	iuce a signai iow	er than the highest	
T	Cut off	32.0 U/Ml					
<u>J</u>	Cut-off	0.5 - 550 U/mL					
K	Analytical Range						
L	Minimum	ADVIA IMS = 0.5 U/mL					
	Detectable	Immuno $1 = 0.9 \text{ U/mL}$					
	Concentration						
M Clinical Results Longitudinal Samples: Two examples of serial patient monitoring studies using Bayer ADVIA IMS assaresults obtained for another marketed device are shown in the following figures: Longitudinal Sample 1							
		140.0	A Second	600.0			
		120.0		500.0		<u> </u>	
		0.00 S C C C C C C C C C C C C C C C C C C	<u> </u>	7 400.0			
		2 80.0		E	1		
		₹ 60.0		300.0 2 200.0	·		
		40.0		¥ 200.0	<u> </u>		
		20.0			1		
		0.0		100.0	—		
		04/15/98 07/24/98	11/01/98 02/09/99	0.0			
		Date		04/05/96 0	8/03/96 12/01/96	03/31/97 07/29/97	
		ADVIA IMS I	mmuno 1		Date		
		10			ADVIA IMS	Immuno 1	
N	Conclusion	Performance of the ADVIA IMS (CΔ 125 II Δecay on a F	Raver ADVIA® IN	ASTM is equivalen	t to the	
- 1	Conclusion	Performance of the ADVIA IMS CA 125 II Assay on a Bayer <i>ADVIA</i> ® IMS [™] is equivalent to the performance of the CA 125 II on he predicate device (Immuno I) and is within proposed specifications. No					
				muno i, and is wi	ann proposed sp	centreations. 140	
	l	safety and effectiveness issues hav	e occii raiseu.				