



Specific Absorption Rate (SAR) Test Report

for

ZTE CORPORATION

on the

GSM Dual-Band Digital Mobile Phone

Report No.	:	FA890205
Trade Name	:	ZTE
Model Name	:	ZTE A933G
FCC ID	:	Q78-ZTEA933G
Date of Testing	:	Sep. 04, 2008
Date of Report	:	Sep. 11, 2008
Date of Review	:	Sep. 11, 2008

- The test results refer exclusively to the tested model/sample only.
- Without written approval of SPORTON INTERNATIONAL INC., the test report shall not be reproduced except in full.
- Report Version: Rev. 02

SPORTON INTERNATIONAL INC.

No. 52, Hwa Ya 1st Rd., Hwa Ya Technology Park, Kwei-Shan Hsiang, Tao Yuan Hsien, Taiwan, R.O.C.





Table of Contents

1.		nent of Compliance	
2.	Admir	nistration Data	2
	2.1	Testing Laboratory	
	2.2	Applicant	2
	2.3	Manufacturer	2
	2.4	Application Details	2
3.	Gener	al Information	3
-	3.1	Description of Device Under Test (DUT)	
	3.2	Basic Description of Accessories	
	3.3	Product Photos	
	3.4	Applied Standards	
	3.5	Device Category and SAR Limits	
	3.6	Test Conditions	
		3.6.1 Ambient Condition	
		3.6.2 Test Configuration	
4.	Specif	fic Absorption Rate (SAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5		leasurement Setup	
υ.	5.1	DASY4 E-Field Probe System	
	0.1	5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 E-Field Probe Calibration	
	5.2	DATA Acquisition Electronics (DAE)	
	5.3	Robot.	9
	5.4	Measurement Server	
	5.5	SAM Twin Phantom	
	5.6	Device Holder for SAM Twin Phantom	
	5.7	Data Storage and Evaluation	
	0.1	5.7.1 Data Storage	
		5.7.2 Data Evaluation	
	5.8	Test Equipment List	
6.		e Simulating Liquids	
7.		tainty Assessment	
		leasurement Evaluation	
8.			
	8.1 8.2	Purpose of System Performance check	
	-	System Setup	
~	8.3	Validation Results	
9.		iption for DUT Testing Position	
10.		Irement Procedures	
	10.1	Spatial Peak SAR Evaluation	
	10.2	Scan Procedures	
	10.3	SAR Averaged Methods	
11.		est Results	
	11.1	Conducted Power	
	11.2	Test Records for Head SAR Test	
	11.3	Test Records for Body SAR Test	
		ences	27
Арр	oendix	A - System Performance Check Data	
Арр	oendix	B - SAR Measurement Data	
Apr	pendix	C - Calibration Data	

Appendix D - Product Photos

Appendix E - Test Setup Photos



1. <u>Statement of Compliance</u>

The Specific Absorption Rate (SAR) maximum results found during testing for the **ZTE CORPORATION GSM Dual-Band Digital Mobile Phone ZTE A933G** are as follows (with expanded uncertainty 21.9%):

SAR	GSM850	GSM1900	
Position	(W/kg)	(W/Kg)	
Head	0.646	1	
Body	0.966	0.403	

They are in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in IEEE C95.3-2002, IEEE P1528-2003, and OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

eey Wi

Roy Wu Manager



2. Administration Data

2.1 <u>Testing Laboratory</u>

Company Name :	SPORTON INTERNATIONAL INC.
Address :	No.52, Hwa-Ya 1 st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,
	TaoYuan Hsien, Taiwan, R.O.C.
Telephone Number :	886-3-327-3456
Fax Number :	886-3-328-4978

2.2 Applicant

Company Name :	ZTE CORPORATION
Address :	ZTE Plaza, Keji Road South, Hi-Tech Industrial Park, Nanshan District,
	Shenzhen, Guangdong, 518057, P.R.China

2.3 Manufacturer

Company Name :	ZTE CORPORATION
Address :	ZTE Plaza, Keji Road South, Hi-Tech Industrial Park, Nanshan District,
	Shenzhen, Guangdong, 518057, P.R.China

2.4 Application Details

Date of reception of application:	Sep. 02, 2008
Start of test :	Sep. 04, 2008
End of test :	Sep. 04, 2008



3. General Information

3.1 <u>Description of Device Under Test (DUT)</u>

Product Feature & Specification				
DUT Type :	UT Type : GSM Dual-Band Digital Mobile Phone			
Trade Name :	ZTE			
Model Name :	ZTE A933G			
FCC ID :	Q78-ZTEA933G			
Tx Frequency :	GSM850 : 824 MHz ~ 849 MHz GSM1900 : 1850 MHz ~1910 MHz			
Rx Frequency :	GSM850 : 869 MHz ~ 894 MHz GSM1900 : 1930 MHz ~ 1990 MHz			
Channel Spacing :	200 KHz			
GPRS Multislot Class :	10			
Maximum Output Power to Antenna : GSM850: 31.52dBm GSM1900: 29.44dBm				
Antenna Type :	Fixed Internal Antenna			
Antenna Gain :	0.74 dBi			
HW Version :	G3yB			
SW Version :	EFS-P108C1(G)V1.0.0B01\\ng3yBV2.0			
Type of Modulation :	GMSK			
DUT Stage :	Production Unit			



3.2 Basic Description of Accessories

Brand Name		ZTE	
	Model Name	STC-A22O50U8-C	
AC Adapter	Power Rating	I/P:100-240Vac, 50-60Hz, 200mA;	
	I ower Kating	O/P: 5Vdc, 700mA	
	AC Power Cord Type	1.8 meter non-shielded cable without ferrite core	
Brand Name		ZTE	
Battery	Model Name	Li3707T42P3h463848	
	Power Rating	3.7Vdc, 720mAh	
Туре		Li-ion	
Brand Name Z		ZTE	
USB Cable Model Name		ZXV100 USB	
Signal Line Type		1.2 meter shielded cable with ferrite core	
LCD Panel	Brand Name	LEAD COMMUNICATIONS LTD.	
Model Name		C17DES01//TM128160E3KFWGWC//CMC-GG1P2042DTSW-W-E	

Remark: Above EUT's information was declared by manufacturer. Please refer to the specifications of manufacturer or User's Manual for more detailed features description.

3.3 Product Photos

Refer to Appendix D.

3.4 <u>Applied Standards</u>

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-2002, IEEE P1528-2003, and OET Bulletin 65 Supplement C (Edition 01-01)



3.5 <u>Device Category and SAR Limits</u>

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user. Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.6 Test Conditions

3.6.1 Ambient Condition

Item	HSL_850	MSL_850	HSL_1900	MSL_1900		
Ambient Temperature (°C)	20-24					
Tissue simulating liquid	21.4°C	21.3°C	21.5°C	21.4°C		
temperature (°C)						
Humidity (%)	<60 %					

3.6.2 Test Configuration

The DUT was set from the emulator to radiate maximum output power during all tests.

The device was controlled by using a base station emulator R&S CMU200. Communication between the device and the emulator was established by air link. The distance between the DUT and the antenna of the emulator is larger than 50 cm and the output power radiated from the emulator antenna is at least 30 dB smaller than the output power of DUT.

Measurements were performed on the lowest, middle, and highest channel for each testing position. Measurements were performed only on the middle channel if the SAR is below 3 dB of limit.

For SAR testing, EUT is in GSM or GPRS link mode. In GSM link mode, its crest factor is 8.3. In GPRS link mode, its crest factor is 4, because EUT is GPRS class 10 device.



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \, \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where is the conductivity of the tissue, is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.





5. SAR Measurement Setup

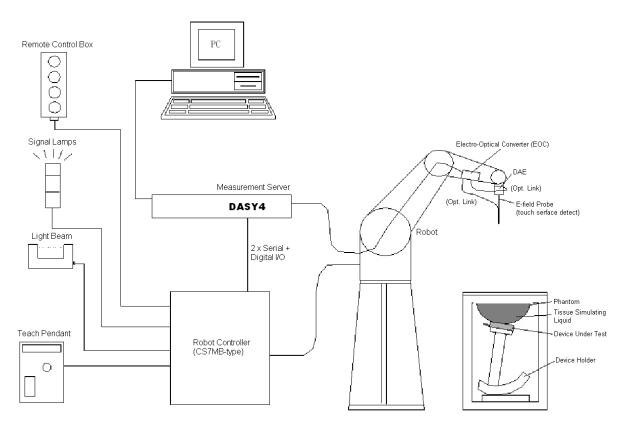


Fig. 5.1 DASY4 System

The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- > A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- A device holder
- Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.



5.1 <u>DASY4 E-Field Probe System</u>

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

Construction	Symmetrical design with triangular core	
	Built-in optical fiber for surface detection system	
	Built-in shielding against static charges	
	PEEK enclosure material (resistant to organic solvents)	
Frequency	10 MHz to 3 GHz	41 2
Directivity	\pm 0.2 dB in brain tissue (rotation around probe axis) \pm 0.4 dB in brain tissue (rotation perpendicular to	
	probe axis)	
Dynamic Range	5 µ W/g to 100mW/g; Linearity: ±0.2dB	
Surface Detection	\pm 0.2 mm repeatability in air and clear liquids on reflecting surface	
Dimensions	Overall length: 330mm Tip length: 16mm	Fig. 5.2 Probe Setup on Robot
	Body diameter: 12mm	Fig. 5.2 I robe Setup on Robot
	Tip diameter: 6.8mm	
	Distance from probe tip to dipole centers: 2.7mm	
Application	General dosimetry up to 3GHz	
	Compliance tests for mobile phones and Wireless	
	LAN	
	Fast automatic scanning in arbitrary phantoms	

5.1.1 ET3DV6 E-Field Probe Specification

5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

Sensitivity	X axis : 1.0	X axis : 1.63 μV		is : 1.66 μV	Z axis : 2.08 µV
Diode compression point		X axis : 92 mV		kis : 96 mV	Z axis : 91 mV
Conversion factor	Frequency (MHz)	X a	xis	Y axis	Z axis
(Head / Body)	800~1000	6.58 / 6.10		6.58 / 6.10	6.58 / 6.10
	1710~1910	5.16 / 4.68		5.16 / 4.68	5.16 / 4.68
Boundary effect	Frequency (MHz)	Alı	oha	Depth	
(Head / Body)	800~1000	0.32	0.36	2.42 / 2.52	
	1710~1910	0.50 /	0.61	2.61 / 2.56	

NOTE: The probe parameters have been calibrated by the SPEAG.



5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

5.3 <u>Robot</u>

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY4 system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- > Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

5.4 <u>Measurement Server</u>

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE4 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



5.5 <u>SAM Twin Phantom</u>

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- ➢ Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

*Water-sugar based liquid

*Glycol based liquids

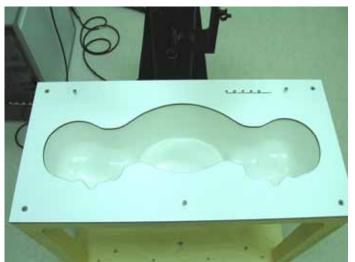


Fig. 5.3 Top View of Twin Phantom



Fig. 5.4 Bottom View of Twin Phantom





5.6 Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY4 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY4 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $_{\rm r}$ =3 and loss tangent δ = 0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



5.7 Data Storage and Evaluation

5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-less media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.7.2 Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm _{<i>i</i>} , a_{i0} , a_{i1} , a_{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	dcpi
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	
	- Density	

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as :

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = compensated signal of channel i (i = x, y, z) U_i = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter) dcp_i = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$ **H-field probes** : $H_i = \sqrt{V_i} \frac{a_{i0+}a_{i1}f + a_{i2}f^2}{f}$ with V_i = compensated signal of channel *i* (*i* = x, y, z) *Norm*_i = sensor sensitivity of channel i (i = x, y, z) $\mu V/(V/m)^2$ for E-field Probes *ConvF* = sensitivity enhancement in solution a_{ii} = sensor sensitivity factors for H-field probes f = carrier frequency [GHz] E_i = electric field strength of channel *i* in V/m H_i = magnetic field strength of channel *i* in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g*Etot* = total field strength in V/m= conductivity in [mho/m] or [Siemens/m] = equivalent tissue density in g/cm^3

* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

 P_{pwe} = equivalent power density of a plane wave in mW/cm² with E_{tot} = total electric field strength in V/m H_{tot} = total magnetic field strength in A/m





5.8 <u>Test Equipment List</u>

Manufacturer	Nome of Fauinment	Tupe/Model	Serial Number	Calibration		
Wanulacturer	Name of Equipment	Type/Model	Serial Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	Aug. 26, 2008	Aug. 25, 2009	
SPEAG	835MHz System Validation Kit	D835V2	499	Mar. 17, 2008	Mar. 16, 2010	
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 28, 2008	Mar. 27, 2010	
SPEAG	Data Acquisition Electronics	DAE4	778	Sep. 17, 2007	Sep. 16, 2008	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1303	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1446	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1383	NCR	NCR	
SPEAG	ELI4 Phantom	QD 0VA 001 BB	1029	NCR	NCR	
SPEAG	Test Arch Phantom	N/A	N/A	NCR	NCR	
SPEAG	Phone Positoiner	N/A	N/A	NCR	NCR	
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR	
SPEAG	Software	DASY4 V4.7 Build 55	N/A	NCR	NCR	
SPEAG	Software	SEMCAD V1.8 Build 176	N/A	NCR	NCR	
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR	
Agilent	PNA Series Network Analyzer	E8358A	US40260131	Apr. 02, 2008	Apr. 01, 2009	
Agilent	Wireless Communication Test Set	E5515C	GB46311322	Dec. 22, 2006	Dec. 21, 2008	
R&S	Universal Radio Communication Tester	CMU200	103937	Oct. 19, 2007	Oct. 18, 2008	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
AR	Power Amplifier	5S1G4M2	0328767	NCR	NCR	
R&S	Power Meter	NRVD	101394	Oct. 31, 2007	Oct. 30, 2008	
R&S	Power Sensor	NRV-Z1	100130	Oct. 31, 2007	Oct. 30, 2008	

Table 5.1 Test Equipment List



6. <u>Tissue Simulating Liquids</u>

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR)or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The following ingredients for tissue simulating liquid are used:

- ▶ Water: deionized water (pure H₂0), resistivity \geq 16MΩ- as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittivity
- Salt: pure NaCl to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- DGMBE: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 – to reduce relative permittivity.

band 850MHZ and	1900 MHz.			
Ingredient	HSL-850	MSL-850	HSL-1900	MSL-1900
Water	532.98 g	631.68 g	552.42 g	716.56 g
Cellulose	0 g	0 g	0 g	0 g
Salt	18.3 g	11.72 g		4.0 g
Preventol D-7	2.4 g	1.2 g	0 g	0 g
Sugar	766.0 g	600.0 g	0 g	0 g
DGMBE		0 g	444.52 g	300.67 g
Total amount	1 liter (1.3 kg)	1 liter (1.3 kg)	1 liter (1.0 kg)	1 liter (1.0 kg)
Dielectric	f = 835 MHz	f=835 MHz	f= 1900 MHz	f= 1900 MHz
Parameters at 22°	$r = 41.5 \pm 5\%$,	$r = 55.2 \pm 5\%$	$\epsilon_{\rm r} = 40.0 \pm 5\%$,	$\epsilon_{\rm r} = 53.3 \pm 5 \%$,
	$= 0.90 \pm 5\%$ S/m	$= 0.97 \pm 5\%$ S/m	σ= 1.4±5% S/m	σ= 1.52±5% S/m

Table 6.1 gives the recipes for one liter of head and body tissue simulating liquid for frequency band 850MHZ and 1900 MHz.

Table 6.1 Recipes for Tissue Simulating Liquid

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.



Band Position		Frequency	Conductivity	Permittivity	Measurement
		(MHz)	(σ)	(E _r)	Date
		824.2	0.887	40.5	
	Head	836.4	0.901	40.6	Sep. 04, 2008
GSM850		848.8	0.91	40.6	
(824 ~ 849 MHz)		824.2	0.967	56.3	
	Body	836.4	0.978	56.3	Sep. 04, 2008
		848.8	0.988	56.1	
		1850.2	1.35	41.9	
	Head	1880.0	1.39	41.8	Sep. 04, 2008
GSM1900		1909.8	1.43	42.0	
(1850 ~ 1910 MHz)		1850.2	1.47	52.2	
	Body	1880.0	1.49	52.2	Sep. 04, 2008
		1909.8	1.53	52.1	

Table 6.2 shows the measuring results for head and muscle simulating liquid.

Table 6.2 Measuring Results for Simulating Liquid

The measuring data are consistent with $_r$ = 41.5±5% and $= 0.9\pm5\%$ for head GSM850, $_r$ = 55.2 $\pm 5\%$ and $= 0.97 \pm 5\%$ for body GSM850, $_r$ = 40.0 $\pm 5\%$ and $= 1.4 \pm 5\%$ for head GSM1900, and $_r$ = 53.3 $\pm 5\%$ and $= 1.52 \pm 5\%$ for body GSM1900.





7. <u>Uncertainty Assessment</u>

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	$_{1/k}$ (b)	1/ 3	1/ 6	1/ 2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

(b) is the coverage factor

Table 7.1 Multiplying Factions for Various Distributions

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.





Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement Equipment						
Probe Calibration	±5.9 %	Normal	1	1	±5.9 %	∞
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	∞
Boundary Effects	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	∞
System Detection Limits	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	±0.8 %	Rectangular	$\sqrt{3}$	1	±0.5 %	∞
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	±1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Probe Positioner	±0.4 %	Rectangular	$\sqrt{3}$	1	±0.2 %	∞
Probe Positioning	±2.9 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Max. SAR Eval.	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9	145
Device Holder	±3.6 %	Normal	1	1	±3.6	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9	∞
Phantom and Setup		·				
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	±1.8	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6	∞
Liquid Permittivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.6	±1.7	∞
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5	∞
Combined Standard					10.0	207
Uncertainty					±10.9	387
Coverage Factor for 95 %		K=2				
Expanded uncertainty					±21.9	
(Coverage factor = 2)					±21.9	

Table 7.2 Uncertainty Budget of DASY4



8. SAR Measurement Evaluation

Each DASY4 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY4 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 <u>Purpose of System Performance check</u>

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 <u>System Setup</u>

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 835 MHz and 1900 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

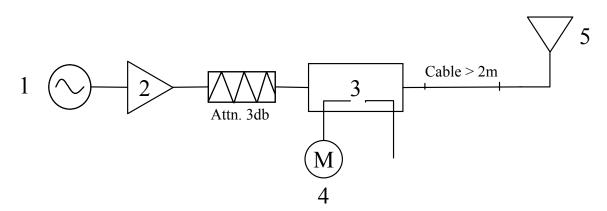


Fig. 8.1 System Setup for System Evaluation



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 835 MHz or 1900 MHz Dipole

The output power on dipole port must be calibrated to 20dBm (100mW) before dipole is connected.



Fig 8.2 Dipole Setup



8.3 Validation Results

Comparing to the original SAR value provided by SPEAG, the validation data should be within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Frequency	Position	SAR	Target (W/kg)	Measurement data (W/kg)	Variation	Measurement Date
925MU	Head	SAR (1g)	9.16	9.91	8.2 %	Sep. 04, 2008
	пеац	SAR (10g)	6.0	6.5	8.3 %	Sep. 04, 2008
835MHz Body	Dodu	SAR (1g)	9.52	10.2	7.1 %	$S_{ap} = 0.4 + 2008$
	Бойу	SAR (10g)	6.37	6.76	6.1 %	Sep. 04, 2008
1900MHz —	Head	SAR (1g)	39.5	39.6	0.3 %	San 04 2008
	пеац	SAR (10g)	20.6	20.7	0.5 %	Sep. 04, 2008
	Dodu	SAR (1g)	40.1	40.8	1.7 %	San 04 2008
	Body	SAR (10g)	21.3	21.5	0.9 %	Sep. 04, 2008

 Table 8.1 Target and Measurement Data Comparison

The table above indicates the system performance check can meet the variation criterion.



9. Description for DUT Testing Position

This DUT was tested in ten different positions. They are as follows:

- 1. Right cheek with close mode
- 2. Right tilted with close mode
- 3. Left cheek with close mode
- 4. Left tilted with close mode
- 5. Right cheek with open mode
- 6. Right tilted with open mode
- 7. Left cheek with open mode
- 8. Left tilted with open mode
- 9. Face with 1.5cm Gap
- 10. Bottom with 1.5cm Gap
- 1) "Cheek Position"
 - i) To position the device with the vertical center line of the body of the device and the horizontal line crossing the center piece in a plane parallel to the sagittal plane of the phantom. While maintaining the device in this plane, align the vertical center line with the reference plane containing the three ear and mouth reference point (M, RE and LE) and align the center of the ear piece with the line RE-LE.
 - ii) To move the device towards the phantom with the ear piece aligned with the line LE-RE until the phone touched the ear. While maintaining the device in the reference plane and maintaining the phone contact with the ear, move the bottom of the phone until any point on the front side is in contact with the cheek of the phantom or until contact with the ear is lost (see Fig. 9.1).

2) "Tilted Position"

- i) To position the device in the "cheek" position described above.
- ii) While maintaining the device the reference plane described above and pivoting against the ear, move it outward away from the mouth by an angle of 15 degrees or until contact with the ear is lost (see Fig. 9.2).

3) "Body Worn"

- i) To position the device parallel to the phantom surface.
- ii) To adjust the phone parallel to the flat phantom.
- iii) To adjust the distance between the EUT surface and the flat phantom to 1.5 cm.

Remark: Please refer to Appendix E for the test setup photos.



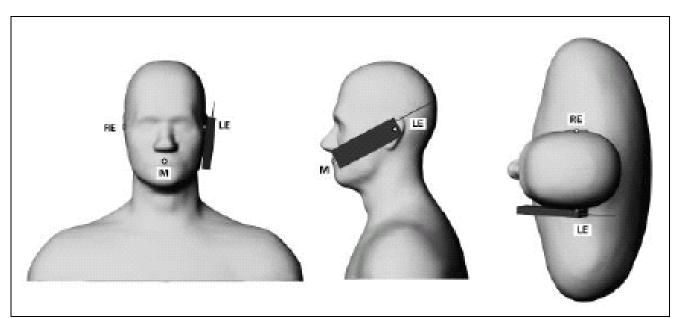


Fig. 9.1 Phone Position 1, "Cheek" or "Touch" Position. The reference points for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.

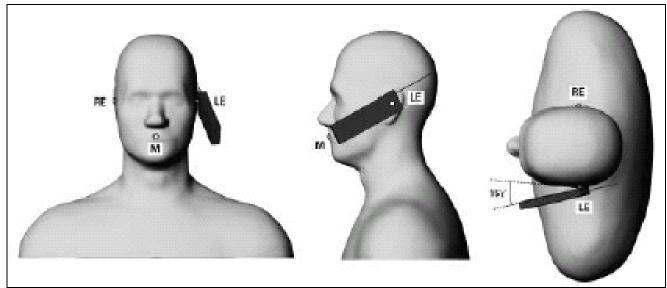


Fig. 9.2 Phone Position 2, "Tilted Position". The reference point for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.



10. Measurement Procedures

The measurement procedures are as follows:

- Linking DUT with base station emulator CMU200 in middle channel
- Setting CMU200 to allow DUT to radiate maximum output power
- Measuring output power through RF cable and power meter
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- > Taking data for the middle channel on each testing position
- Finding out the largest SAR result on these testing positions of each band
- Measuring output power and SAR results for the low and high channels in this worst case testing position

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- > Power reference measurement

10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, IEEE P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.



The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

10.2 <u>Scan Procedures</u>

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan measures 5x5x7 points with step size 8, 8 and 5 mm. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3 SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



11. SAR Test Results

11.1 Conducted Power

Band Mode Channel		GSM 850 (dBm)		GSM 1900 (dBm)			
	128	189	128	189	128	189	
GSM	31.52	31.47	31.48	29.4	29.12	28.82	
GPRS 8	31.52	31.47	31.49	29.44	29.16	28.85	
GPRS 10	31.48	31.43	31.46	29.38	29.11	28.83	

11.2 Test Records for Head SAR Test

EUT Mode	Position	Band	Chan.	Freq. (MHz)	Modulation Type	Measured 1g SAR (W/kg)	Power Drift	Limit (W/kg)	Result
Close	Right Cheek	GSM850	189	836.4	GMSK	0.275	-0.11	1.6	Pass
Close	Right Tilted	GSM850	189	836.4	GMSK	0.14	0.01	1.6	Pass
Close	Left Cheek	GSM850	189	836.4	GMSK	0.231	-0.194	1.6	Pass
Close	Left Tilted	GSM850	189	836.4	GMSK	0.129	-0.05	1.6	Pass
Open	Right Cheek	GSM850	189	836.4	GMSK	0.604	-0.124	1.6	Pass
Open	Right Tilted	GSM850	189	836.4	GMSK	0.326	0.009	1.6	Pass
Open	Left Cheek	GSM850	189	836.4	GMSK	0.575	0.005	1.6	Pass
Open	Left Tilted	GSM850	189	836.4	GMSK	0.305	-0.077	1.6	Pass
Open	Right Cheek	GSM850	128	824.2	GMSK	0.512	0.129	1.6	Pass
Open	Right Cheek	GSM850	251	848.8	GMSK	0.646	-0.121	1.6	Pass
Close	Right Cheek	GSM1900	661	1880.0	GMSK	1	-0.136	1.6	Pass
Close	Right Tilted	GSM1900	661	1880.0	GMSK	0.278	0.03	1.6	Pass
Close	Left Cheek	GSM1900	661	1880.0	GMSK	0.854	-0.105	1.6	Pass
Close	Left Tilted	GSM1900	661	1880.0	GMSK	0.24	-0.011	1.6	Pass
Open	Right Cheek	GSM1900	661	1880.0	GMSK	0.393	0.102	1.6	Pass
Open	Right Tilted	GSM1900	661	1880.0	GMSK	0.148	0.193	1.6	Pass
Open	Left Cheek	GSM1900	661	1880.0	GMSK	0.401	-0.197	1.6	Pass
Open	Left Tilted	GSM1900	661	1880.0	GMSK	0.111	0.13	1.6	Pass
Close	Right Cheek	GSM1900	512	1850.2	GMSK	0.893	-0.147	1.6	Pass
Close	Right Cheek	GSM1900	810	1909.8	GMSK	0.978	-0.027	1.6	Pass
Close	Left Cheek	GSM1900	512	1850.2	GMSK	0.764	-0.086	1.6	Pass
Close	Left Cheek	GSM1900	810	1909.8	GMSK	0.843	0.088	1.6	Pass

11.3 Test Records for Body SAR Test

Position	Band	Chan.	Freq. (MHz)	Modulation Type	Measured 1g SAR (W/kg)	Power Drift	Limit (W/kg)	Result
Bottom with 1.5cm Gap	GSM850	189	836.4	GMSK	0.378	-0.13	1.6	Pass
Face with 1.5cm Gap	GSM850	189	836.4	GMSK	0.217	-0.107	1.6	Pass
Bottom with 1.5cm Gap	GSM850	128	824.2	GMSK	0.403	-0.124	1.6	Pass
Bottom with 1.5cm Gap	GSM850	251	848.8	GMSK	0.349	0.008	1.6	Pass
Bottom with 1.5cm Gap	GSM1900	661	1880.0	GMSK	0.966	-0.117	1.6	Pass
Face with 1.5cm Gap	GSM1900	661	1880.0	GMSK	0.462	-0.194	1.6	Pass
Bottom with 1.5cm Gap	GSM1900	512	1850.2	GMSK	0.789	-0.126	1.6	Pass
Bottom with 1.5cm Gap	GSM1900	810	1909.8	GMSK	0.832	-0.002	1.6	Pass

Remark: Test Engineer : Gordon Lin, Jason Wang, and Eric Huang



12.<u>References</u>

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DASY4 System Handbook



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/9/4

System Check_Head_835MHz

DUT: Dipole 835 MHz

Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium: HSL_850 Medium parameters used: f = 835 MHz; $\sigma = 0.899$ mho/m; $\varepsilon_r = 40.6$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.4 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.09 mW/g

 $\begin{array}{l} \textbf{Pin=100mW/Zoom Scan (7x7x7)/Cube 0: } Measurement grid: dx=5mm, dy=5mm, dz=5mm \\ Reference Value = 35.9 V/m; Power Drift = -0.081 dB \\ Peak SAR (extrapolated) = 1.44 W/kg \\ \textbf{SAR(1 g) = 0.991 mW/g; SAR(10 g) = 0.650 mW/g} \\ Maximum value of SAR (measured) = 1.08 mW/g \end{array}$

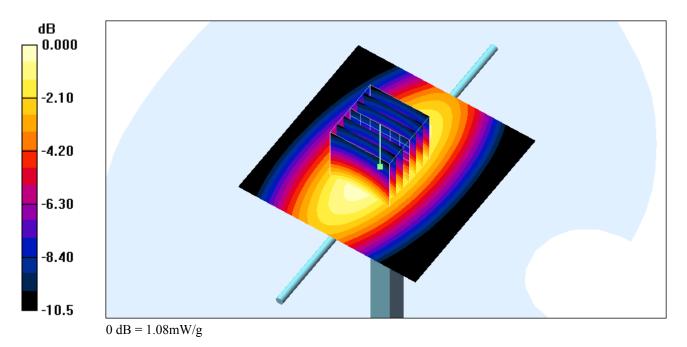





Date: 2008/9/4

System Check_Head_1900MHz

DUT: Dipole 1900 MHz


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: HSL_1900 Medium parameters used: f = 1900 MHz; $\sigma = 1.42$ mho/m; $\epsilon_r = 41.9$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 4.74 mW/g

 $\label{eq:product} \begin{array}{l} \textbf{Pin=100mW/Zoom Scan (7x7x7)/Cube 0:} \ \text{Measurement grid: } dx=5mm, dy=5mm, dz=5mm \\ \text{Reference Value} = 58.3 \ \text{V/m; Power Drift} = 0.001 \ \text{dB} \\ \text{Peak SAR (extrapolated)} = 7.26 \ \text{W/kg} \\ \textbf{SAR(1 g)} = \textbf{3.96 mW/g; SAR(10 g)} = \textbf{2.07 mW/g} \\ \text{Maximum value of SAR (measured)} = 4.42 \ \text{mW/g} \end{array}$

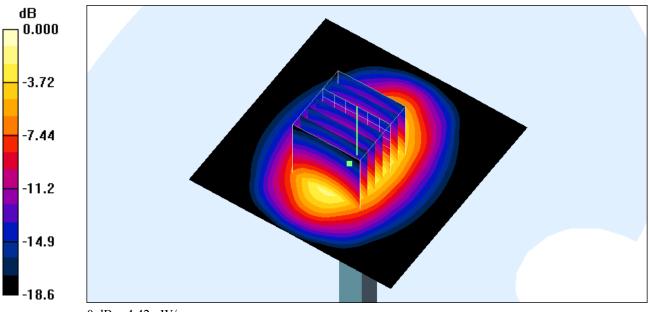

 $0 \, dB = 4.42 \, mW/g$





Date: 2008/9/4

System Check_Body_835MHz

DUT: Dipole 835 MHz


Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 835 MHz; $\sigma = 0.977$ mho/m; $\epsilon_r = 56.3$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.3 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (41x41x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (interpolated) = 0.996 mW/g

 $\label{eq:product} \begin{array}{l} \textbf{Pin=100mW/Zoom Scan (7x7x7)/Cube 0:} \ \text{Measurement grid: } dx=5mm, dy=5mm, dz=5mm \\ \text{Reference Value} = 31.8 \ \text{V/m; Power Drift} = -0.023 \ \text{dB} \\ \text{Peak SAR (extrapolated)} = 1.43 \ \text{W/kg} \\ \textbf{SAR(1 g)} = \textbf{1.02 mW/g; SAR(10 g)} = \textbf{0.676 mW/g} \\ \text{Maximum value of SAR (measured)} = 1.10 \ \text{mW/g} \end{array}$

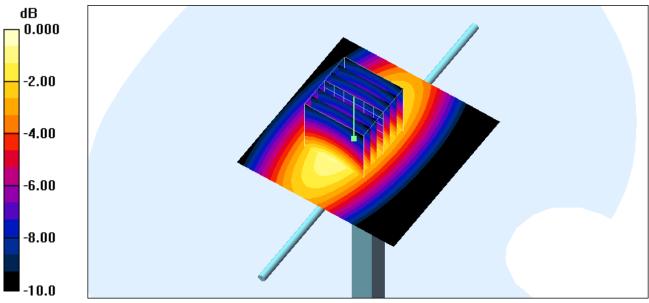

0 dB = 1.10 mW/g





Date: 2008/9/4

System Check_Body_1900MHz

DUT: Dipole 1900 MHz


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1900 MHz; σ = 1.52 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature : 23.1 ; Liquid Temperature : 21.4

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.65 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.6 V/m; Power Drift = -0.011 dB Peak SAR (extrapolated) = 7.47 W/kg **SAR(1 g) = 4.08 mW/g; SAR(10 g) = 2.15 mW/g** Maximum value of SAR (measured) = 4.60 mW/g

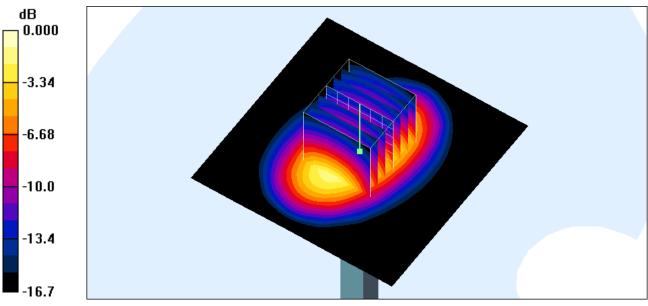

 $0 \, dB = 4.60 \, mW/g$



Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/9/4

Right Cheek_GSM850 Ch251_Open

DUT: 890205

Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:8.3 Medium: HSL_850 Medium parameters used: f = 849 MHz; $\sigma = 0.91$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.4 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch251/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.697 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.3 V/m; Power Drift = -0.121 dB Peak SAR (extrapolated) = 0.874 W/kg SAR(1 g) = 0.646 mW/g; SAR(10 g) = 0.457 mW/g Maximum value of SAR (measured) = 0.697 mW/g

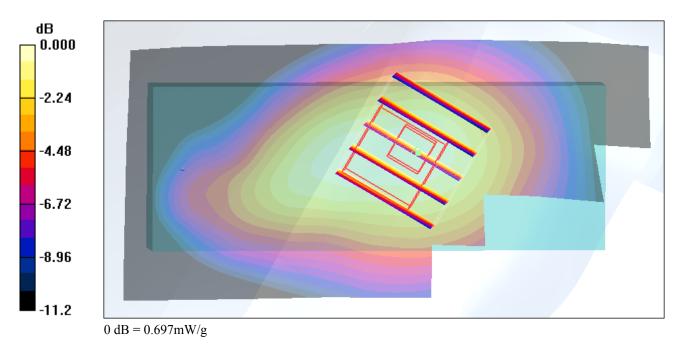



Date: 2008/9/4

Right Tilted_GSM850 Ch189_Open

DUT: 890205

Communication System: GSM850; Frequency: 836.4 MHz;Duty Cycle: 1:8.3 Medium: HSL_850 Medium parameters used: f = 836.4 MHz; $\sigma = 0.901$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.4 °C


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch189/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.344 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 17.2 V/m; Power Drift = 0.009 dBPeak SAR (extrapolated) = 0.413 W/kgSAR(1 g) = 0.326 mW/g; SAR(10 g) = 0.235 mW/gMaximum value of SAR (measured) = 0.347 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 17.2 V/m; Power Drift = 0.009 dB Peak SAR (extrapolated) = 0.479 W/kgSAR(1 g) = 0.264 mW/g; SAR(10 g) = 0.172 mW/gMaximum value of SAR (measured) = 0.306 mW/g

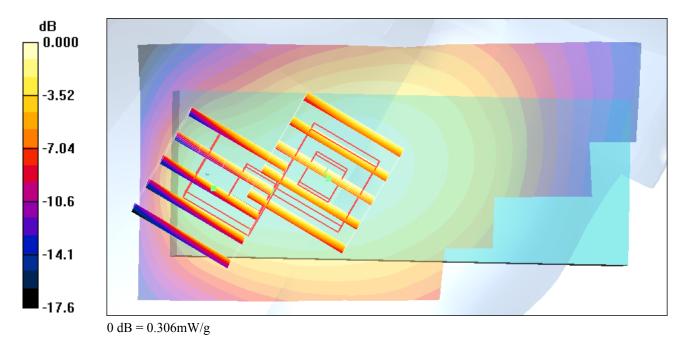



Date: 2008/9/4

Left Tilted_GSM850 Ch189_Open

DUT: 890205

Communication System: GSM850; Frequency: 836.4 MHz;Duty Cycle: 1:8.3 Medium: HSL_850 Medium parameters used: f = 836.4 MHz; $\sigma = 0.901$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.4 °C


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch189/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.314 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 17.4 V/m; Power Drift = -0.077 dB Peak SAR (extrapolated) = 0.385 W/kg SAR(1 g) = 0.305 mW/g; SAR(10 g) = 0.220 mW/g Maximum value of SAR (measured) = 0.326 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 17.4 V/m; Power Drift = -0.077 dBPeak SAR (extrapolated) = 0.435 W/kgSAR(1 g) = 0.261 mW/g; SAR(10 g) = 0.171 mW/gMaximum value of SAR (measured) = 0.289 mW/g

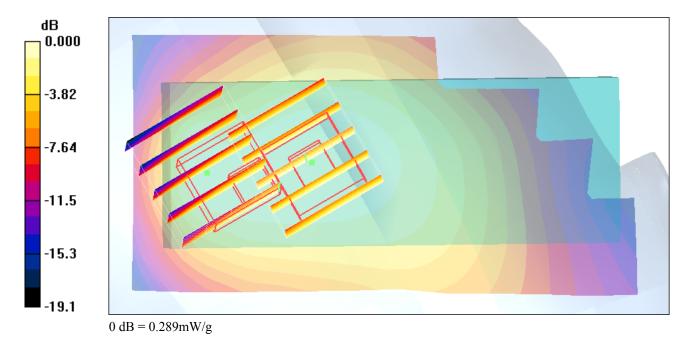



Date: 2008/9/4

Left Cheek_GSM850 Ch189_Open

DUT: 890205

Communication System: GSM850; Frequency: 836.4 MHz;Duty Cycle: 1:8.3 Medium: HSL_850 Medium parameters used: f = 836.4 MHz; $\sigma = 0.901$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.8 °C; Liquid Temperature : 21.4 °C


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch189/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.625 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.1 V/m; Power Drift = 0.005 dB Peak SAR (extrapolated) = 0.771 W/kg SAR(1 g) = 0.575 mW/g; SAR(10 g) = 0.403 mW/g Maximum value of SAR (measured) = 0.617 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.1 V/m; Power Drift = 0.005 dB Peak SAR (extrapolated) = 0.769 W/kg SAR(1 g) = 0.546 mW/g; SAR(10 g) = 0.394 mW/g Maximum value of SAR (measured) = 0.612 mW/g

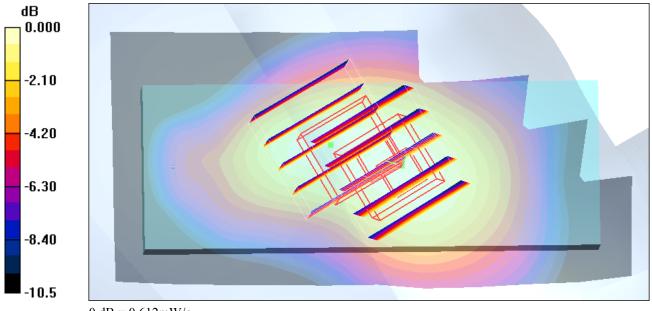

0 dB = 0.612 mW/g



Date: 2008/9/4

Right Cheek_GSM1900 Ch661_Close

DUT: 890205

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.39$ mho/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.05 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.1 V/m; Power Drift = -0.136 dB Peak SAR (extrapolated) = 1.78 W/kg SAR(1 g) = 1 mW/g; SAR(10 g) = 0.574 mW/g Maximum value of SAR (measured) = 1.09 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.1 V/m; Power Drift = -0.136 dB Peak SAR (extrapolated) = 1.69 W/kg SAR(1 g) = 0.927 mW/g; SAR(10 g) = 0.522 mW/g Maximum value of SAR (measured) = 1.08 mW/g

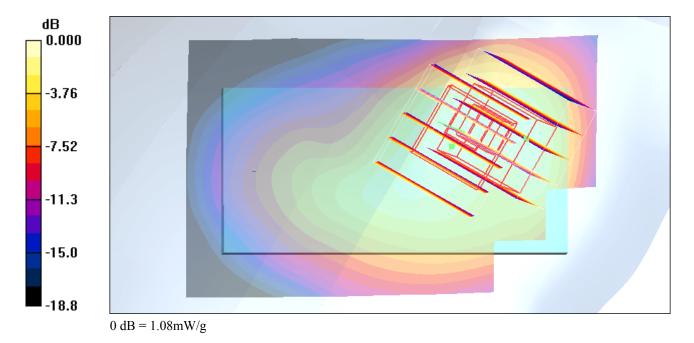



Date: 2008/9/4

Right Tilted GSM1900 Ch661 Close

DUT: 890205


Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:8.3 Medium: HSL 1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.39 \text{ mho/m}$; $\varepsilon_r = 41.8$; $\rho = 1000 \text{ kg/m}^3$ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.306 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.7 V/m; Power Drift = 0.030 dBPeak SAR (extrapolated) = 0.434 W/kgSAR(1 g) = 0.278 mW/g; SAR(10 g) = 0.171 mW/gMaximum value of SAR (measured) = 0.290 mW/g

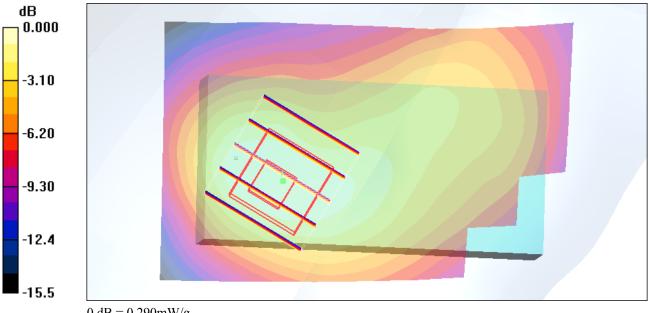

 $0 \, dB = 0.290 \, mW/g$





Date: 2008/9/4

Left Cheek_GSM1900 Ch661_Close

DUT: 890205

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.39$ mho/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.9 ; Liquid Temperature : 21.5


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.978 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 9.53 V/m; Power Drift = -0.105 dB Peak SAR (extrapolated) = 1.40 W/kg SAR(1 g) = 0.854 mW/g; SAR(10 g) = 0.511 mW/g Maximum value of SAR (measured) = 0.935 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 9.53 V/m; Power Drift = -0.105 dB Peak SAR (extrapolated) = 1.44 W/kg SAR(1 g) = 0.842 mW/g; SAR(10 g) = 0.518 mW/g Maximum value of SAR (measured) = 0.940 mW/g

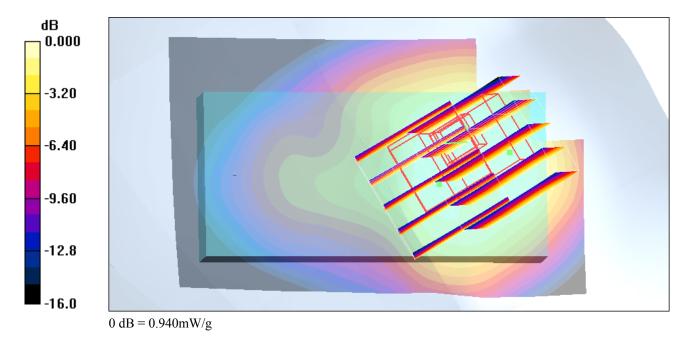



Date: 2008/9/4

Left Tilted_GSM1900 Ch661_Close

DUT: 890205


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.39 mho/m; ϵ_r = 41.8; ρ = 1000 kg/m³ Ambient Temperature : 22.6 ; Liquid Temperature : 21.5

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.270 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 12.3 V/m; Power Drift = -0.011 dB Peak SAR (extrapolated) = 0.378 W/kg SAR(1 g) = 0.240 mW/g; SAR(10 g) = 0.145 mW/g Maximum value of SAR (measured) = 0.260 mW/g

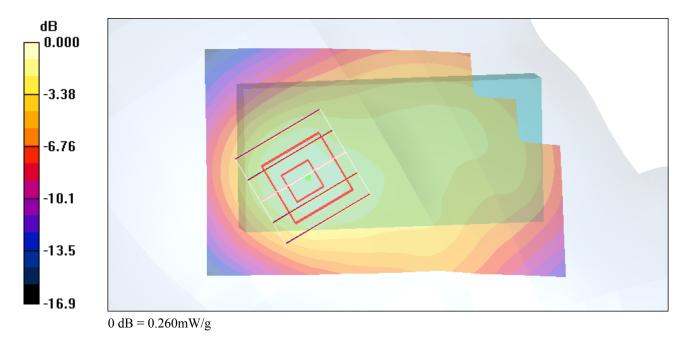



Date: 2008/9/4

Body_GSM850 Ch189_Face with 1.5cm Gap_GPRS10

DUT: 890205

Communication System: GSM850; Frequency: 836.4 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used : f = 836.4 MHz; $\sigma = 0.978$ mho/m; $\epsilon_r = 56.3$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.5 ; Liquid Temperature : 21.3

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)


- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch189/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.233 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.45 V/m; Power Drift = -0.107 dBPeak SAR (extrapolated) = 0.271 W/kgSAR(1 g) = 0.217 mW/g; SAR(10 g) = 0.158 mW/gMaximum value of SAR (measured) = 0.231 mW/g

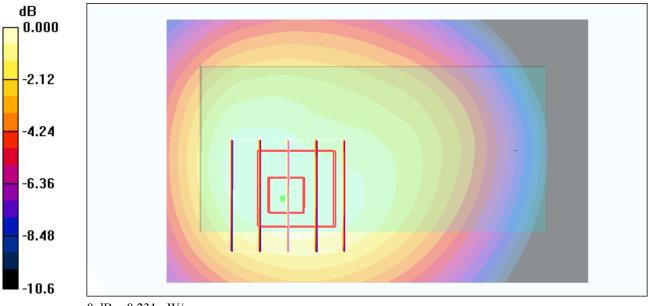

0 dB = 0.231 mW/g





Date: 2008/9/4

Body_GSM850 Ch128_Bottom with 1.5cm Gap_GPRS10

DUT: 890205

Communication System: GSM850; Frequency: 824.2 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used : f = 824.2 MHz; $\sigma = 0.967$ mho/m; $\epsilon_r = 56.3$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.5 ; Liquid Temperature : 21.3

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)


- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch128/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.435 mW/g

Ch128/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.19 V/m; Power Drift = -0.124 dB Peak SAR (extrapolated) = 0.539 W/kg SAR(1 g) = 0.403 mW/g; SAR(10 g) = 0.275 mW/g Maximum value of SAR (measured) = 0.433 mW/g

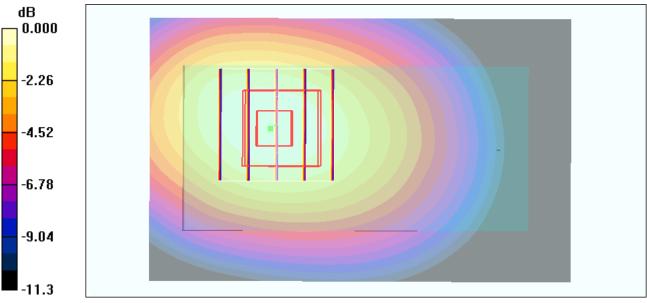

0 dB = 0.433 mW/g





Date: 2008/9/4

Body_GSM1900 Ch661_Front with 1.5cm Gap_GPRS10

DUT: 890205

Communication System: PCS 1900; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.49$ mho/m; $\varepsilon_r = 52.2$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.6 ; Liquid Temperature : 21.4

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)


- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.505 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.4 V/m; Power Drift = -0.194 dB Peak SAR (extrapolated) = 0.751 W/kg SAR(1 g) = 0.462 mW/g; SAR(10 g) = 0.281 mW/g Maximum value of SAR (measured) = 0.502 mW/g

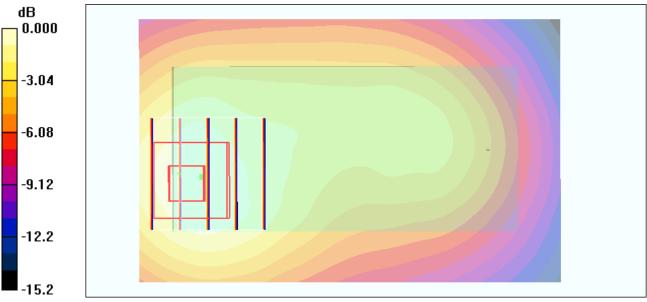

0 dB = 0.502 mW/g





Date: 2008/9/4

Body_GSM1900 Ch661_Bottom with 1.5cm Gap_GPRS10

DUT: 890205

Communication System: PCS 1900; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.49$ mho/m; $\varepsilon_r = 52.2$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.8 ; Liquid Temperature : 21.4

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)


- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.08 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 9.34 V/m; Power Drift = -0.117 dB Peak SAR (extrapolated) = 1.66 W/kg SAR(1 g) = 0.966 mW/g; SAR(10 g) = 0.546 mW/g Maximum value of SAR (measured) = 1.05 mW/g

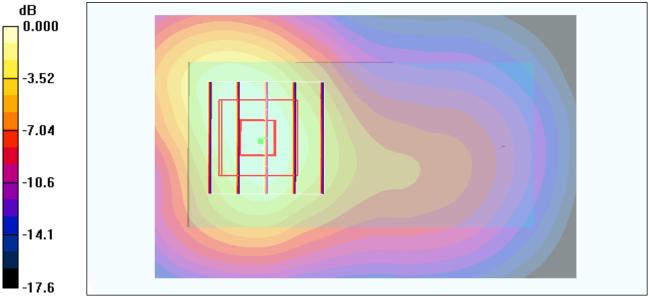

0 dB = 1.05 mW/g



Date: 2008/9/4

Right Cheek_GSM850 Ch251_Open_2D

DUT: 890205


Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:8.3 Medium: HSL_850 Medium parameters used: f = 849 MHz; σ = 0.91 mho/m; ϵ_r = 40.6; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.4

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.06, 6.06, 6.06); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch251/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mmMaximum value of SAR (interpolated) = 0.697 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.3 V/m; Power Drift = -0.121 dB Peak SAR (extrapolated) = 0.874 W/kg SAR(1 g) = 0.646 mW/g; SAR(10 g) = 0.457 mW/g Maximum value of SAR (measured) = 0.697 mW/g

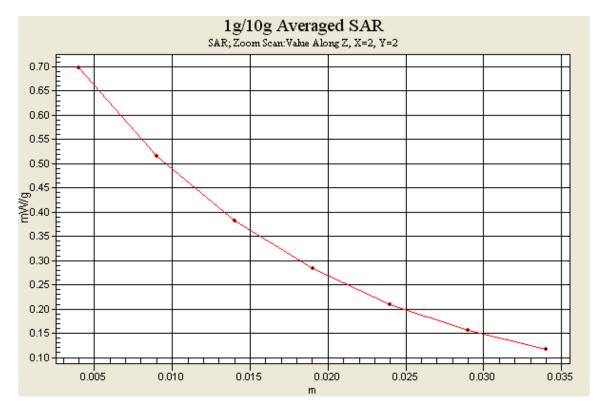



Date: 2008/9/4

Right Cheek_GSM1900 Ch661_Close_2D

DUT: 890205


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.39$ mho/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.01, 5.01, 5.01); Calibrated: 2008/8/26

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.05 mW/gCh661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.1 V/m; Power Drift = -0.136 dBPeak SAR (extrapolated) = 1.78 W/kgSAR(1 g) = 1 mW/g; SAR(10 g) = 0.574 mW/gMaximum value of SAR (measured) = 1.09 mW/gCh661/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.1 V/m; Power Drift = -0.136 dBPeak SAR (extrapolated) = 1.69 W/kgSAR(1 g) = 0.927 mW/g; SAR(10 g) = 0.522 mW/gMaximum value of SAR (measured) = 1.08 mW/g

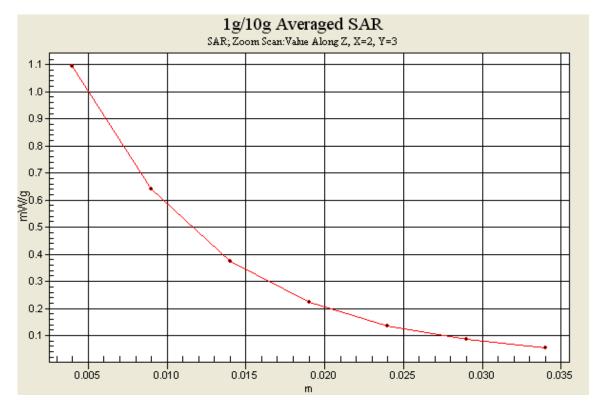



Test Report No : FA890205

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/9/4

Body_GSM850 Ch128_Bottom with 1.5cm Gap_GPRS10_2D

DUT: 890205

Communication System: GSM850; Frequency: 824.2 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used : f = 824.2 MHz; $\sigma = 0.967$ mho/m; $\epsilon_r = 56.3$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.4 ; Liquid Temperature : 21.3

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26


- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch128/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.435 mW/g

Ch128/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.19 V/m; Power Drift = -0.124 dB Peak SAR (extrapolated) = 0.539 W/kg SAR(1 g) = 0.403 mW/g; SAR(10 g) = 0.275 mW/g Maximum value of SAR (measured) = 0.433 mW/g

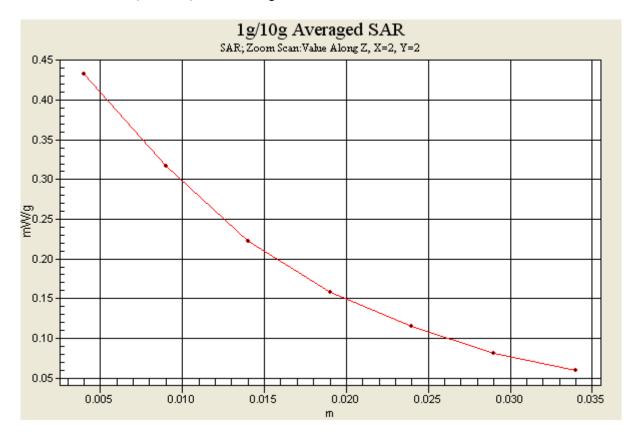



Date: 2008/9/4

Body_GSM1900 Ch661_Bottom with 1.5cm Gap_GPRS10_2D

DUT: 890205

Communication System: PCS 1900; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.49 mho/m; ϵ_r = 52.2; ρ = 1000 kg/m³

Ambient Temperature : 22.8 ; Liquid Temperature : 21.4

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26


- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (51x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.08 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 9.34 V/m; Power Drift = -0.117 dB Peak SAR (extrapolated) = 1.66 W/kg SAR(1 g) = 0.966 mW/g; SAR(10 g) = 0.546 mW/g Maximum value of SAR (measured) = 1.05 mW/g

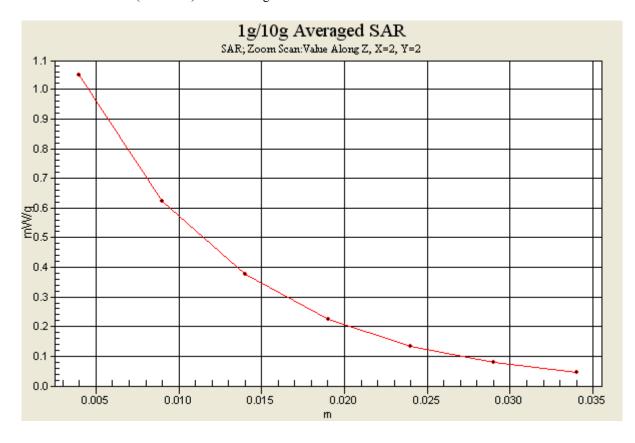



Appendix C – Calibration Data

Test Report No : FA890205

Calibration Laboratory of SWISS Schweizerischer Kalibrierdienst s Schmid & Partner Service suisse d'étalonnage С ac-MR Engineering AG Servizio svizzero di taratura s Zeughausstrasse 43, 8004 Zurich, Switzerland BRD Swiss Calibration Service Accreditation No.: SCS 108 Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Certificate No: D835V2-499 Mar08 Sporton (Auden) Client CALIBRATION CERTIFICATE D835V2 - SN: 499 Object QA CAL-05.v7 Calibration procedure(s) Calibration procedure for dipole validation kits March 17, 2008 Calibration date: Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) ID# Cal Date (Calibrated by, Certificate No.) Primary Standards Scheduled Calibration Power meter EPM-442A GB37480704 04-Oct-07 (METAS, No. 217-00736) Oct-08 Power sensor HP 8481A US37292783 04-Oct-07 (METAS, No. 217-00736) Oct-08 SN: 5086 (20g) 07-Aug-07 (METAS, No 217-00718) Reference 20 dB Attenuator Aug-08 Reference Probe ES3DV2 SN: 3025 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) Mar-09 DAF4 SN 909 03-Sep-07 (SPEAG, No. DAE4-909 Sep07) Sep-08 ID # Secondary Standards Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (SPEAG, in house check Oct-07) In house check: Oct-09 04-Aug-99 (SPEAG, in house check Oct-07) RF generator R&S SMT-06 100005 in house check: Oct-09 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (SPEAG, in house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Claudio Leubler Laboratory Technician Katia Pokovic Approved by: Technical Manager Issued: March 17, 2008 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-499_Mar08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



CR RIATO

S

С

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-499_Mar08

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	41
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.90 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.29 mW / g
SAR normalized	normalized to 1W	9.16 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.16 mW / g ± 17.0 % (k=2)
	aandillan	
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	1.50 mW/g
Republication and the second		1.50 mW / g 6.00 mW / g

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 3 of 9



Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.0 ± 6 %	1.00 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.46 mW/g
SAR normalized	normalized to 1W	9.84 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	9.52 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.63 mW/g
SAR normalized	normalized to 1W	6.52 mW/g
SAR for nominal Body TSL parameters 2	normalized to 1W	6.37 mW / g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.9 Ω - 2.3 jΩ
Return Loss	- 28.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.2 Ω - 3.3 jΩ
Return Loss	- 29.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.392 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 10, 2003

Certificate No: D835V2-499_Mar08

Page 5 of 9



DASY4 Validation Report for Head TSL

Date/Time: 17.03.2008 11:32:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499


Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: HSL 900 MHz; Medium parameters used: f = 835 MHz; $\sigma = 0.9$ mho/m; $\epsilon_r = 41.5$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(6.09, 6.09, 6.09); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Unnamed procedure/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.9 V/m; Power Drift = -0.005 dB Peak SAR (extrapolated) = 3.34 W/kg SAR(1 g) = 2.29 mW/g; SAR(10 g) = 1.5 mW/g Maximum value of SAR (measured) = 2.58 mW/g

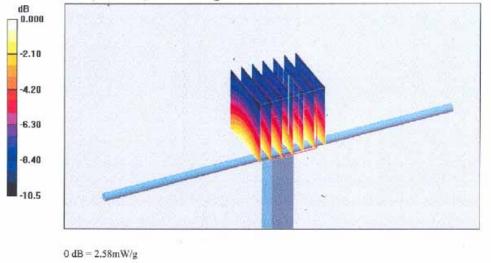

Certificate No: D835V2-499_Mar08

Page 6 of 9



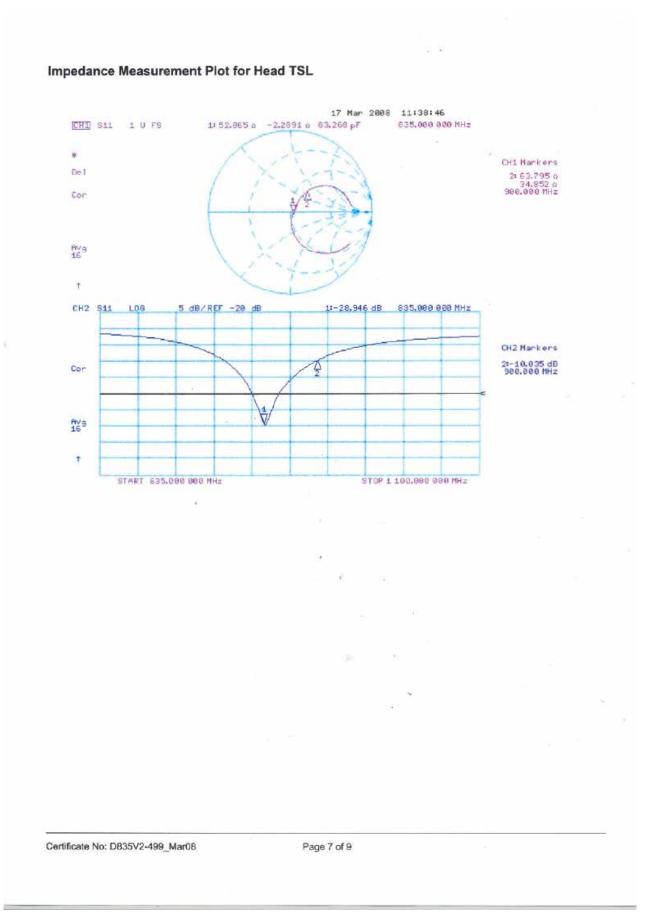

©2008 SPORTON INTERNATIONAL INC. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



DASY4 Validation Report for Body TSL

Date/Time: 10.03.2008 12:48:36

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499


Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: MSL900; Medium parameters used: f = 835 MHz; $\sigma = 1$ mho/m; $\varepsilon_r = 54$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(5.85, 5.85, 5.85); Calibrated: 01.03.2008
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW, d = 15 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 51.8 V/m; Power Drift = 0.036 dB Peak SAR (extrapolated) = 3.59 W/kg SAR(1 g) = 2.46 mW/g; SAR(10 g) = 1.63 mW/g Maximum value of SAR (measured) = 2.64 mW/g

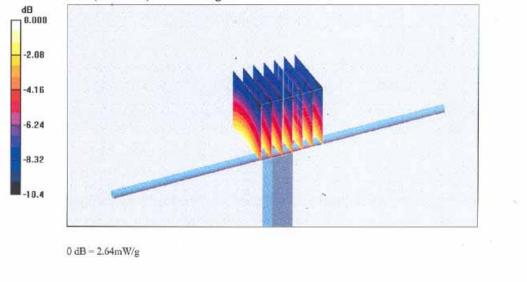


Certificate No: D835V2-499_Mar08

Page 8 of 9



Impedance Measurement Plot for Body TSL

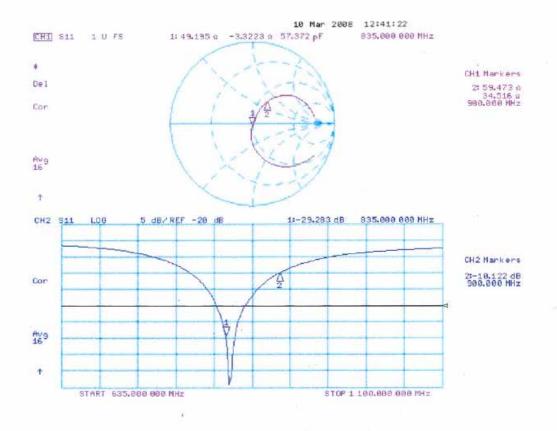

Certificate No: D835V2-499_Mar08

Page 9 of 9



Test Report No : FA890205

eughausstrasse 43, 8004 Zuric	h, Switzerland		chweizerischer Kalibrierdienst ervice suisse d'étalonnage ervizio svizzero di taratura wiss Calibration Service
Accredited by the Swiss Federal (The Swiss Accreditation Servic Aultilateral Agreement for the r	e is one of the signatorie	es to the EA	.: SCS 108
Client Sporton (Aude			01900V2-5d041_Mar08
CALIBRATION	CERTIFICATE		
Object	D1900V2 - SN: 5	id041	
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	edure for dipole validation kits	
Calibration date:	March 18, 2008		
Condition of the calibrated item	In Tolerance	n de fan inder de ferste ander	
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physical units o robability are given on the following pages and ar ny facility: environment temperature (22 ± 3)°C an	e part of the certificate.
The measurements and the unce All calibrations have been condu	rtainties with confidence protection of the closed laborator	robability are given on the following pages and ar	e part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&	rtainties with confidence protection of the closed laborator	robability are given on the following pages and an ny facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.)	e part of the certificate.
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A	rtainties with confidence protected in the closed laborator TE official for calibration)	robability are given on the following pages and an ny facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%, Scheduled Calibration Oct-08
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C an <u>Cal Date (Calibrated by, Certificate No.)</u> 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%, Scheduled Calibration Oct-08 Oct-08
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	rtainties with confidence p cted in the closed laborator TE ortical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 07-Aug-07 (METAS, No 217-00718)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2	rtainties with confidence p cted in the closed laborator TE ortical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID #	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID # MY41092317	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID # MY41092317 100005	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08 In house check: Oct-09
The measurements and the unce	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID # MY41092317	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5087.2 (10r) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 GB37480704	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08 In house check: Oct-09 In house check: Oct-08 Oct-08
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter EPM-442A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 GB37480704 Name	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736) Function	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08 In house check: Oct-09 In house check: Oct-08
The measurements and the unce All calibrations have been condui Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter EPM-442A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5087.2 (10r) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 GB37480704	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08 In house check: Oct-09 In house check: Oct-08 Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 GB37480704 Name	robability are given on the following pages and ar ry facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736) Function	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Aug-08 Mar-09 Sep-07 Scheduled Check In house check: Oct-08 In house check: Oct-09 In house check: Oct-08 Oct-08

Certificate No: D1900V2-5d041_Mar08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

С

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d041_Mar08

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.47 mho/m ± 6 %
Head TSL temperature during test	(21.1 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	10.1 mW/g
SAR normalized	normalized to 1W	40.4 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	39.5 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.20 mW / g
SAR normalized	normalized to 1W	20.8 mW/g
SAR for nominal Head TSL parameters 1	normalized to 1W	20.6 mW / g ± 16.5 % (k=2)

4

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 3 of 9

2.33

Body TSL parameters

The following	parameters and	calculations	were applied.	
---------------	----------------	--------------	---------------	--

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.6 ± 6 %	1.57 mho/m ± 6 %
Body TSL temperature during test	(21.4±0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.4 mW / g
SAR normalized	normalized to 1W	41.6 mW/g
SAR for nominal Body TSL parameters 2	normalized to 1W	40.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.44 mW / g
SAR normalized	normalized to 1W	21.8 mW/g
SAR for nominal Body TSL parameters ²	normalized to 1W	21.3 mW / g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.0 Ω + 5.1 jΩ	
Return Loss	- 24.2 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.0 Ω + 6.1 jΩ
Return Loss	- 23.6 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 04, 2003

Certificate No: D1900V2-5d041_Mar08

Page 5 of 9



DASY4 Validation Report for Head TSL

Date/Time: 18.03.2008 12:05:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: HSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.47 mho/m; ϵ_r = 40.2; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.9, 4.9, 4.9); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 91.7 V/m; Power Drift = 0.013 dB Peak SAR (extrapolated) = 19.1 W/kg SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.2 mW/g Maximum value of SAR (measured) = 11.8 mW/g

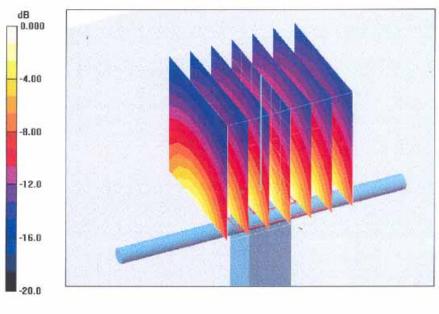


0 dB = 11.8mW/g

Certificate No: D1900V2-5d041_Mar08

Page 6 of 9



Impedance Measurement Plot for Head TSL

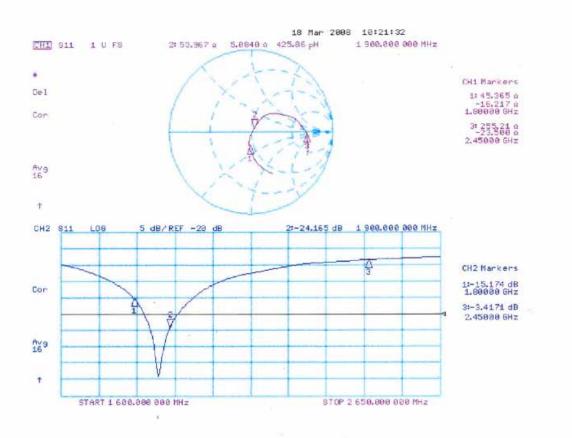

Certificate No: D1900V2-5d041_Mar08

Page 7 of 9



DASY4 Validation Report for Body TSL

Date/Time: 14.03.2008 13:22:24

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.57 mho/m; ϵ_r = 51.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.5, 4.5, 4.5); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 89.7 V/m; Power Drift = 0.004 dB Peak SAR (extrapolated) = 18.6 W/kg SAR(1 g) = 10.4 mW/g; SAR(10 g) = 5.44 mW/g Maximum value of SAR (measured) = 12.0 mW/g

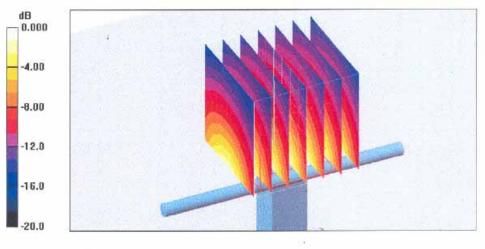


0 dB = 12.0mW/g

Certificate No: D1900V2-5d041 Mar08

Page 8 of 9



Impedance Measurement Plot for Body TSL

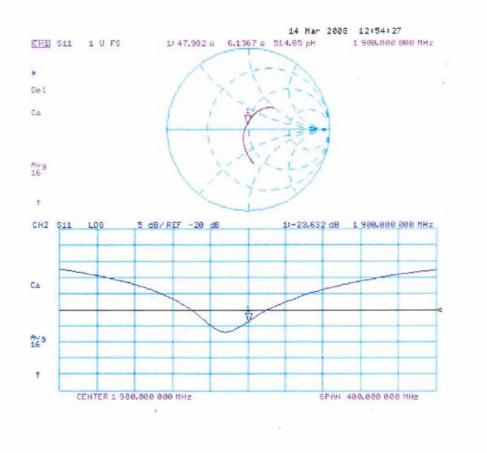

Certificate No: D1900V2-5d041_Mar08

Page 9 of 9



Test Report No : FA890205

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SHISS C NO NO C RUBRATO S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

CALIBRATION CE	(Auoten)	Certificate No:	
ALIBRATION C	RIFICATE		
Object	DAE4 - SD 000 D	04 BG - SN: 778	
Calibration procedure(s)	QA CAL-06.v12 Calibration procee	dure for the data acquisition electro	onics (DAE)
Calibration date:	September 17, 20	07	
Condition of the calibrated item	In Tolerance		
The measurements and the uncerta All calibrations have been conducte	inties with confidence pro	nel standards, which realize the physical units coability are given on the following pages and a v facility: environment temperature (22 ± 3)°C a	are part of the certificate.
Calibration Equipment used (M&TE	chucai for calibration)		
	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Primary Standards Fluke Process Calibrator Type 702	ID # SN: 6295803	13-Oct-06 (Elcal AG, No: 5492)	Oct-07
Primary Standards Fluke Process Calibrator Type 702	ID #		and an other statements and statements and
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	ID # SN: 6295803	13-Oct-06 (Elcal AG, No: 5492)	Oct-07
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ID # SN: 6295803 SN: 0810276	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	Oct-07 Oct-07
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID # SN: 6295803 SN: 0810278 ID #	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	Oct-07 Oct-07 Scheduled Check
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ID # SN: 6295803 SN: 0810278 ID #	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	Oct-07 Oct-07 Scheduled Check
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ID # SN: 6295803 SN: 0810278 ID #	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	Oct-07 Oct-07 Scheduled Check
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ID # SN: 6295803 SN: 0810276 ID # SE UMS 006 AB 1004	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house) 25-Jun-07 (SPEAG, in house check)	Oct-07 Oct-07 Scheduled Check In house check Jun-08
Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID # SN: 6295803 SN: 0810276 ID # SE UMS 006 AB 1004	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-96 (Elcal AG, No: 5478) Check Date (in house) 25-Jun-07 (SPEAG, in house check) Function	Oct-07 Oct-07 Scheduled Check In house check Jun-08

Certificate No: DAE4-778_Sep07

Page 1 of 5



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



GWISS CP ZO PF/BRATT

S

Schweizerischer Kallbrierdienst Service suisse d'étalonnage

C Service suisse d etaionnage

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
- Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
- Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
- Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
- Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-778_Sep07

Page 2 of 5

DC Voltage Measurement

High Range:	1LSB =	6.1µV ,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV

Calibration Factors	X	Y	z
High Range	404.715 ± 0.1% (k=2)	403.520 ± 0.1% (k=2)	405.065 ± 0.1% (k=2)
Low Range	3.99539 ± 0.7% (k=2)	3.96323 ± 0.7% (k=2)	3.97102 ± 0.7% (k=2)

Connector Angle

이 이 이 이 이 이 이 이 이 이 이 이 이 이 이 이 이 이 이	35 C 2 2 C 3 a 1 C 1 a - 1 C 2 a -
Connector Angle to be used in DASY system	309 ° ± 1 °

Certificate No: DAE4-778_Sep07

Page 3 of 5



Appendix

1. DC Voltage Linearity

High Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	200000	199999.5	0.00
Channel X + Input	20000	20004.41	0.02
Channel X - Input	20000	-20002.56	0.01
Channel Y + Input	200000	200000.3	0.00
Channel Y + Input	20000	20003.67	0.02
Channel Y - Input	20000	-20003.41	0.02
Channel Z + Input	200000	200000.3	0.00
Channel Z + Input	20000	20002.49	0.01
Channel Z - Input	20000	-20006.25	0.03

Low Range	Input (μV)	Reading (µV)	Error (%)
Channel X + Input	2000	1999.9	0.00
Channel X + Input	200	199.47	-0.26
Channel X - Input	200	-200.56	0.28
Channel Y + Input	2000	2000.1	0.00
Channel Y + Input	200	199.15	-0.43
Channel Y - Input	200	-200.77	0.39
Channel Z + Input	2000	2000	0.00
Channel Z + Input	200	199.22	-0.39
Channel Z - Input	200	-201.39	0.69

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	-6.00	-6.42
	- 200	7.17	6.60
Channel Y	200	-2.49	-2.64
	- 200	2.04	1.25
Channel Z	200	-10.83	-10.80
	- 200	9.19	. 8.80

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	<u> </u>	2.57	0.15
Channel Y	200	0.11	-	4.08
Channel Z	200	-1.80	1.03	1

Certificate No: DAE4-778_Sep07

Page 4 of 5

a 13



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16068	16321
Channel Y	16180	16239
Channel Z	16405	16167

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10M\Omega$

11	Average (µV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-0.14	-1.23	0.61	0.34
Channel Y	-0.85	-2.24	0.48	0.49
Channel Z	-1.24	-2.43	0.38	0.51

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	201.7
Channel Y	0.2000	201.7
Channel Z	0.1999	202.5

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)		
Supply (+ Vcc)	(ð.)	+7.9	
Supply (- Vcc)		-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	≠ +6 ·	+14
Supply (- Vcc)	-0.01	-8	-9

Page 5 of 5



Test Report No : FA890205

Engineering AG ughausstrasse 43, 8004 Zurio	ch, Switzerland	HOC MRA	Service suisse d'étaionnage Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accredit the Swiss Accreditation Servic	e is one of the signatori	es to the EA	No.: SCS 108
luitilateral Agreement for the r	ana a nnean ann an		o: ET3-1787_Aug08
CALIBRATION	22.50	E	
Dbject	ET3DV6 - SN:1	787	
Calibration procedure(s)	Concession of the second second second	and QA CAL-23.v3 redure for dosimetric E-field probe	S
Calibration date:	August 26, 2008	B; () () () () () () () () () () () () ()	
Condition of the calibrated item	In Tolerance		
The measurements and the unor	ertainties with confidence	itional standards, which realize the physical un probability are given on the following pages at ory facility: environment temperature $(22 \pm 3)^{4}$	are part of the certificate.
The measurements and the unco	ertainties with confidence	probability are given on the following pages at long facility: environment temperature $(22 \pm 3)^{11}$	are part of the certificate.
he measurements and the unor a calibrations have been condu alibration Equipment used (M&	ertainties with confidence	probability are given on the following pages at long facility: environment temperature $(22 \pm 3)^{11}$	are part of the certificate.
he measurements and the unor il calibrations have been condu alibration Equipment used (M& rimary Standards	ertainties with confidence cted in the closed laborat TE ontical for calibration)	probability are given on the following pages at lory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788)	Id are part of the certificate. C and humidity < 70% Scheduled Calibration Apr-09
he measurements and the unor 8 calibrations have been condu alibration Equipment used (M& rimary Standards ower metar E4419B ower sensor E4412A	ertainties with confidence cted in the closed laborat TE ortical for calibration) ID # GB41293874 MY41495277	probability are given on the following pages at lory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09
he measurements and the unor al calibrations have been condu- alibration Equipment used (M& nimary Standards ower metar E4419B ower sensor E4412A ower sensor E4412A	etainties with confidence cted in the closed laborat TE ortical for calibration) ID # GB41293874 MY41495277 MY41498087	probability are given on the following pages at lory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	Id are part of the certificate. C and humidity < 70%⊨ Scheduled Calibration Apr-09 Apr-09 Apr-09
The measurements and the unor al calibrations have been condu- calibration Equipment used (M& Inimary Standards lower metar E44198 lower sensor E4412A lower sensor E4412A leference 3 dB Attenuator	ettainties with confidence cted in the closed laborat TE ortical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c)	probability are given on the following pages at ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788)	Id are part of the certificate. C and humidity < 70%⊨ Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ettainties with confidence cted in the closed laborat TE ortical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5056 (20b)	probability are given on the following pages at ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 31-Mar-08 (No. 217-00787)	Id are part of the certificate. C and humidity < 70%⊨ Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Apr-09
The measurements and the unor all calibrations have been condu- calibration Equipment used (M& Primary Standards Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator	ettainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41495277 MY41498067 SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b)	probability are given on the following pages at ony facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786)	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09
he measurements and the unor al calibrations have been condu- alibration Equipment used (M& mmary Standards ower meter E4419B ower sensor E4412A elerence 3 dB Attenuator leference 3 dB Attenuator leference 30 dB Attenuator leference 30 dB Attenuator leference 90 dB Attenuator	ettainties with confidence cted in the closed laborat TE ortical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5056 (20b)	probability are given on the following pages at ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 31-Mar-08 (No. 217-00787)	Id are part of the certificate. C and humidity < 70%⊨ Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Apr-09
The measurements and the unor No calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator	ettainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b) SN: 3013	probability are given on the following pages at ony facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00786) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. ES3-3013_Jan08)	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09
The measurements and the unor all calibrations have been condu- calibration Equipment used (M& Inimary Standards lower meter E44198 lower sensor E44198 lower sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 9 Tobe ES3DV2 (AE4	ettainties with confidence cted in the closed laborat TE ontical for calibration) ID # GB41293874 MY41495277 MY41495077 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5129 (30b) SN: 3013 SN: 660	probability are given on the following pages ar ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00786) 1-Apr-08 (No. 217-00786) 1-Apr-08 (No. 217-00786) 1-Jul-08 (No. 217-00786) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jam-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07)	Id are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jan-09 Jan-09 Sep-08
The measurements and the unor KI calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 70 bB Attenuator Reference Frobe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ettainties with confidence cted in the closed laborat TE ontical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5129 (30b) SN: \$513 SN: 660 ID #	probability are given on the following pages at ony facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1.Apr-08 (No. 217-00786) 1.Apr-08 (No. 217-00786) 1.Jul-08 (No. 217-00786) 1.Jul-08 (No. 217-00786) 31-Mar-08 (No. 217-00786) 3.Jul-08 (No. 217-00787) 1.Jul-08 (No. 217-00866) 2.Jun-08 (No. ES3-3013_Jan08) 3.Sep-07 (No. DAE4-660_Sep07) Check Date (In house)	Id are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check
The measurements and the unor all calibrations have been condu- calibration Equipment used (M& Animary Standards Power sensor E44198 Power sensor E4412A Nover sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30	ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41495277 MY41498067 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b) SN: \$	probability are given on the following pages ar ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 1-Jul-08 (No. 217-00865) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check In house check: Cct-09
The measurements and the unor all calibrations have been condu- calibration Equipment used (M& Animary Standards Power sensor E44198 Power sensor E4412A Nover sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30	ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b) SN: \$5129 (30b) SN: \$5129 (30b) SN: \$600 ID # US3642U01700 US37390585	probability are given on the following pages ar lory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00865) 2-Jan-08 (No. 217-00865) 2-Jan-08 (No. 237-00865) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07)	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jan-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
The measurements and the unor	ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41495277 MY41498067 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b) SN: \$	probability are given on the following pages ar ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 1-Jul-08 (No. 217-00865) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jan-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
The measurements and the unor Na calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 70 d	ertainties with confidence cted in the closed laborat TE ontical for calibration) ID # GB41293874 MY41495087 SN: \$5054 (3c) SN: \$5056 (20b) SN: \$	probability are given on the following pages ar ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00786) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00865) 2-Jan-08 (No. 217-00865) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	Id are part of the certificate. C and humidity < 70%: Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jan-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



CRIVER Z

S

С

Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization o	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a
 flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787_Aug08

Page 2 of 9





August 26, 2008

Probe ET3DV6

SN:1787

Manufactured: Last calibrated: Recalibrated: May 28, 2003 August 28, 2007 August 26, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1787_Aug08

Page 3 of 9

August 26, 2008

Diode Compression^B

90 mV

93 mV

92 mV

DCP X

DCP Y

DCP Z

3.7 mm 4.7 mm 11.3

3.7 mm 4.7 mm 10.1

0.8

0.8

7.5

0.5

6.5

0.6



ET3DV6 SN:1787

DASY - Parameters of Probe: ET3DV6 SN:1787 Sensitivity in Free Space^A µV/(V/m)2 NormX 1.63 ± 10.1% NormY 1.67 ± 10.1% $\mu V/(V/m)^2$ $\mu V/(V/m)^2$ NormZ 2.18 ± 10.1% Sensitivity in Tissue Simulating Liquid (Conversion Factors) Please see Page 8. Boundary Effect TSL 900 MHz Typical SAR gradient: 5 % per mm Sensor Center to Phantom Surface Distance SAR ... [%] Without Correction Algorithm SARbe [%] With Correction Algorithm TSL 1750 MHz Typical SAR gradient: 10 % per mm Sensor Center to Phantom Surface Distance SAR_{ba} [%] Without Correction Algorithm SAR ... [%] With Correction Algorithm Sensor Offset

Probe Tip to Sensor Center

2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

* The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).

* Numerical linearization parameter: uncertainty not required.

Certificate No: ET3-1787_Aug08


Page 4 of 9



August 26, 2008

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

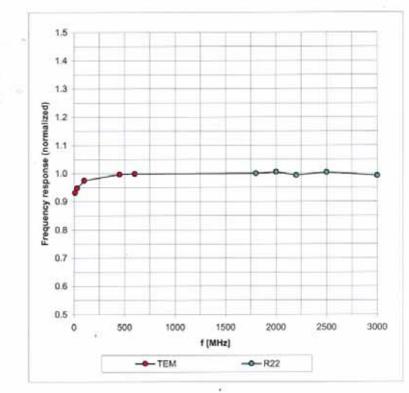


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ET3-1787_Aug08


Page 5 of 9



August 26, 2008

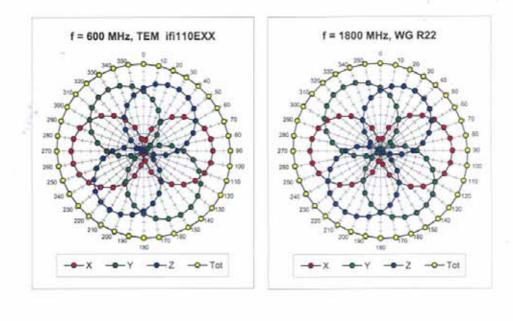

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

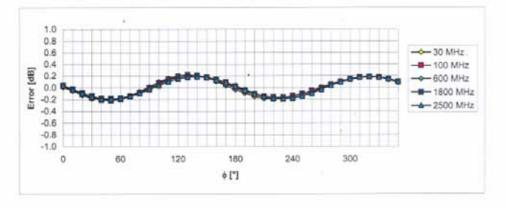

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1787 Aug08


Page 6 of 9



......

ET3DV6 SN:1787

August 26, 2008

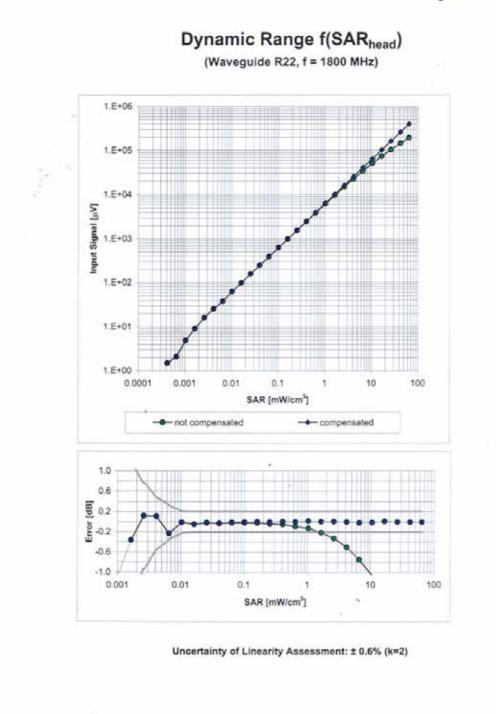


Certificate No: ET3-1787_Aug08

Page 7 of 9



August 26, 2008

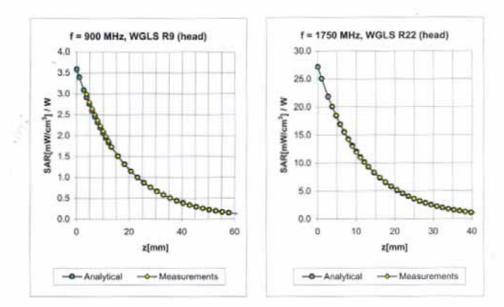

Conversion Factor Assessment

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5±5%	0.97 ± 5%	0.30	2.80	6.06 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.53	2.11	5.36 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	$1.40\pm5\%$	0.59	1.96	5.01 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1,80 ± 5%	0.77	1.57	4.49 ± 11.0% (k=2)
				12.1			
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.31	2.98	5.91 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	$53.4\pm5\%$	1.49 ± 5%	0.60	2.20	4.73 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	$1.52\pm5\%$	0.68	1.95	4.49 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.90	1.51	3.79 ± 11.0% (k=2)

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1787_Aug08


Page 8 of 9



August 26, 2008

Deviation from Isotropy in HSL

Error (\, \,), f = 900 MHz

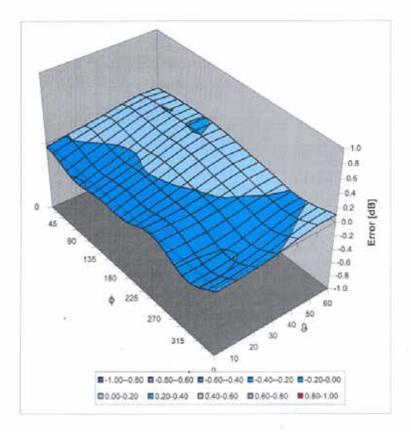

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1787_Aug08

Page 9 of 9



Test Report No : FA890205




Appendix D - Product Photos






Appendix E - Test Setup Photos

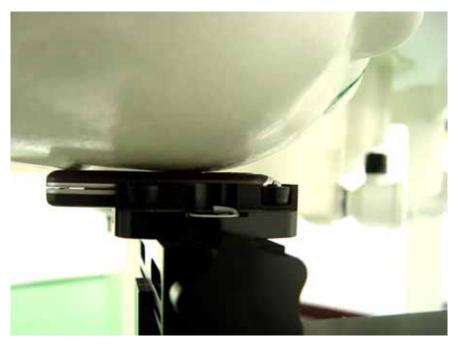

Right Cheek with Close Mode

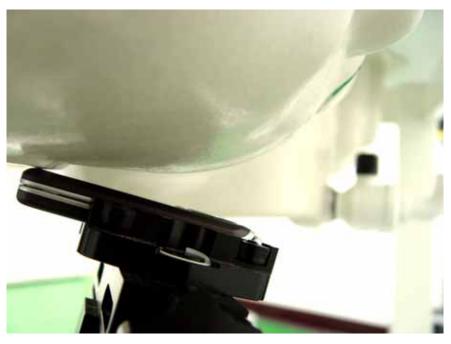


Right Tilted with Close Mode






Left Cheek with Close Mode

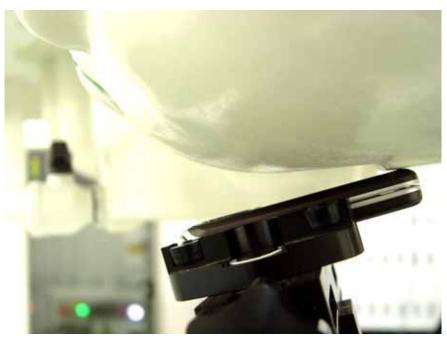

Left Tilted with Close Mode



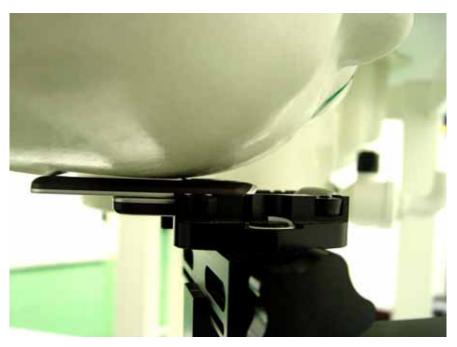


Right Cheek with Open Mode




Right Tilted with Open Mode



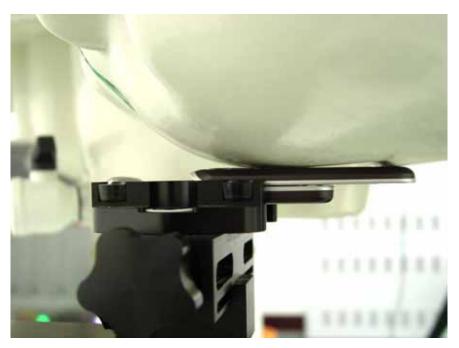


Left Cheek with Open Mode

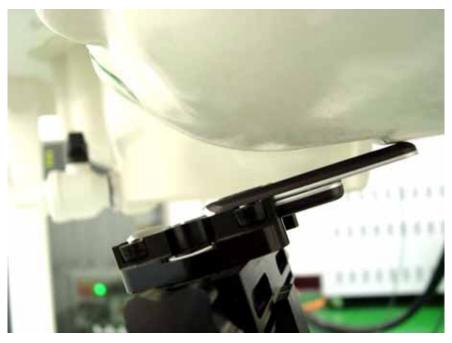

Left Tilted with Open Mode



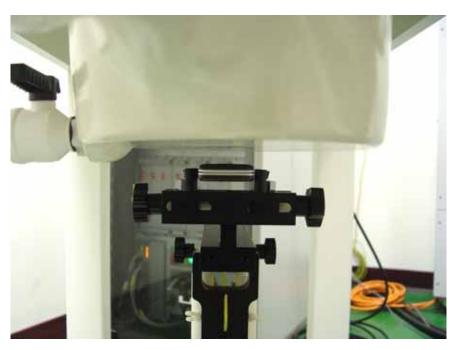

Face with 1.5cm Gap



Bottom with 1.5cm Gap